



Featured Application: Mycotoxins in Peanut Powder on Raptor Biphenyl


5.5 Minute LC-MS/MS Analysis of Mycotoxins in Peanut Powder

- Fast analysis for higher sample throughput.
- Excellent separation improves accuracy for 12 regulated mycotoxins.
- Quick and easy sample preparation (dilute-filter-shoot).

Certain fungi that can grow on agricultural products produce toxic metabolites known as mycotoxins. Modern food processing procedures cannot completely remove these compounds if they are present, so strict monitoring protocols have been established. Although a universal method for the analysis of mycotoxins would allow highly efficient screening, it is very challenging to develop such a method due to differences in physicochemical properties of mycotoxins, extraction efficiencies, and matrix effects. Zhang et al. published a multi-lab study [1] aimed at providing labs with an analytical procedure that could be broadly applied to the analysis of a variety of mycotoxins in many different matrices. Using that work as inspiration, we developed the following LC-MS/MS method that resolves 12 FDA regulated mycotoxins within the pressure limits of traditional HPLC instruments.

In this example, mycotoxins were analyzed in a peanut powder matrix. The use of a relatively short column format, the selectivity of the Biphenyl stationary phase, and the efficiency of 2.7 μm Raptor superficially porous particles provided excellent separations in a fast 5.5 minute analysis (total cycle time of 7 minutes). A coeluting matrix compound that shared the most abundant MRM transition for mycotoxin HT-2 (447.3-285.3) was observed, so a less abundant transition (447.3-345.3) was selected for quantitation. To increase sensitivity, an ammonium buffer was used to promote better ionization of mycotoxins. The Raptor Biphenyl column worked very well for the 12 mycotoxins studied in the cited work, but for longer compound lists containing isobaric mycotoxins with similar structures, the Raptor FluoroPhenyl phase may be necessary to provide adequate chromatographic resolution. The selectivity of the Raptor Fluorophenyl column is demonstrated in an analysis of 20 mycotoxins that can be found by visiting www.restek.com and entering LC_FS0511 in the search.

This method showed excellent precision and accuracy for the 12 FDA regulated mycotoxins that were evaluated during a validation study that covered a variety of matrices (including multiple sources of cornmeal and brown rice flour, in addition to the peanut powder example shown here). Restek would like to thank Dr. Zhang for his technical support during this project.

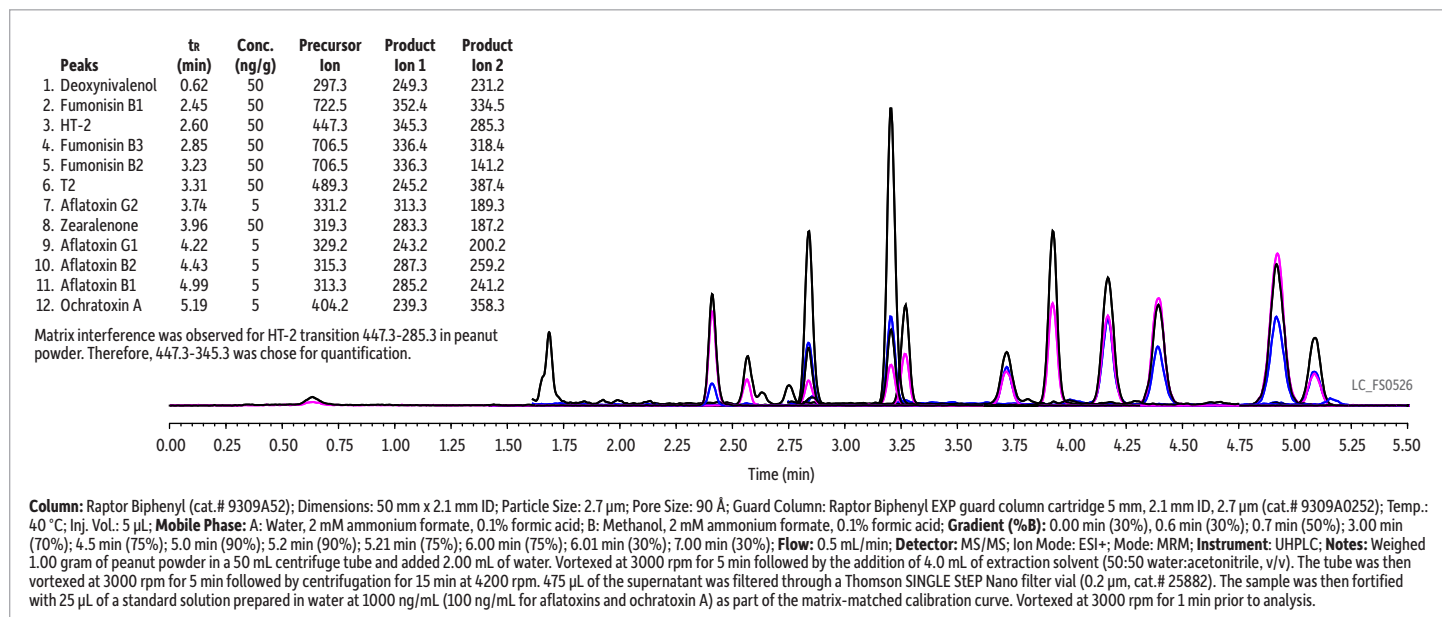

References

1. K. Zhang, M.R. Schaab, G. Southwood, E.R. Tor, L.S. Aston, W. Song, B. Eitzer, S. Majumdar, T. Lapainis, H. Mai, K. Tran, A. El-Demerdash, V. Vega, Y. Cai, J.W. Wong, A.J. Krynitsky, T.H. Begley, A collaborative study: determination of mycotoxins in corn, peanut butter, and wheat flour using stable isotope dilution assay (SIDA) and liquid chromatography-tandem mass spectrometry (LC-MS/MS), *Journal of Agricultural and Food Chemistry*, 65 (33) (2017) 7138-7152. <https://www.ncbi.nlm.nih.gov/pubmed/27983809>.

Raptor Biphenyl LC Columns (USP L11)

Length	2.1 mm cat.#	3.0 mm cat.#	4.6 mm cat.#
1.8 µm Columns			
30 mm	9309232	—	—
50 mm	9309252	930925E	—
100 mm	9309212	930921E	—
150 mm	9309262	—	—
2.7 µm Columns			
30 mm	9309A32	9309A3E	9309A35
50 mm	9309A52	9309A5E	9309A55
100 mm	9309A12	9309A1E	9309A15
150 mm	9309A62	9309A6E	9309A65
5 µm Columns			
30 mm	—	930953E	—
50 mm	9309552	930955E	9309555
100 mm	9309512	930951E	9309515
150 mm	9309562	930956E	9309565
250 mm	—	—	9309575



Raptor EXP Guard Column Cartridges

- Free-Turn architecture lets you change cartridges by hand without breaking inlet/outlet fluid connections—no tools needed.
- Patented titanium hybrid ferrules can be installed repeatedly without compromising high-pressure seal.
- Auto-adjusting design provides ZDV (zero dead volume) connection to any 10-32 female port.

Description	Particle Size	qty.	5 x 2.1 mm cat.#	5 x 3.0 mm cat.#	5 x 4.6 mm cat.#
Raptor Biphenyl EXP Guard Column Cartridge	UHPLC	3-pk.	9309U0252	9309U0253	
Raptor Biphenyl EXP Guard Column Cartridge	2.7 µm	3-pk.	9309A0252	9309A0253	9309A0250
Raptor Biphenyl EXP Guard Column Cartridge	5 µm	3-pk.	930950252	930950253	930950250

Maximum cartridge pressure: 1,034 bar/15,000 psi* (UHPLC), 600 bar/8,700 psi (2.7 µm); 400 bar/5,800 psi (5 µm)

* For maximum lifetime, recommended maximum pressure for UHPLC particles is 830 bar/12,000 psi.

Hybrid Ferrule U.S. Patent No. 8201854, EXP Holders U.S. Patent No. 8696902, EXP2 Wrench U.S. Patent No. D766055. Other U.S. and Foreign Patents Pending. The EXP, Free-Turn, and the Opti- prefix are registered trademarks of Optimize Technologies, Inc.




EXP Direct Connect Holder

Description	qty.	cat.#
EXP Direct Connect Holder for EXP Guard Cartridges (includes hex-head fitting & 2 ferrules)	ea.	25808

Maximum holder pressure: 20,000 psi (1,400 bar)

Hybrid Ferrule U.S. Patent No. 8201854, EXP Holders U.S. Patent No. 8696902, EXP2 Wrench U.S. Patent No. D766055. Other U.S. and Foreign Patents Pending. The EXP, Free-Turn, and the Opti- prefix are registered trademarks of Optimize Technologies, Inc.

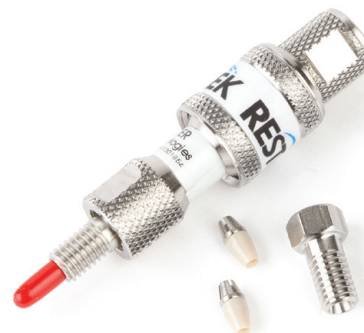

Questions? Contact us or your local Restek representative (www.restek.com/contact-us).

Restek patents and trademarks are the property of Restek Corporation. (See www.restek.com/Patents-Trademarks for full list.) Other trademarks in Restek literature or on its website are the property of their respective owners. Restek registered trademarks are registered in the U.S. and may also be registered in other countries. To unsubscribe from future Restek communications or to update your preferences, visit www.restek.com/subscribe To update your status with an authorized Restek distributor or instrument channel partner, please contact them directly.

© 2019 Restek Corporation. All rights reserved. Printed in the U.S.A.